


Technical specifications

Intended use	Expansion			
Indications for use	Crest expansion			
Description	Conical expansion tip marked every 2 mm (2-4-6-8)			
Tip type	Expander			
Allergenic factor	Tip made of surgical stainless steel as per ASTM F899 - 12b			
	Surgical stainless steel contains: <ul style="list-style-type: none">• nickel• chromium			
Commercial reference	CS6 II : F87566			
Medical class	Class of medical device: IIa according to 93/42/EEC directive			
Adjustments	Ultrasonic generators	Maximum mode	Maximum fine setting	Irrigation
	Implant Center II Piezotome 2 Piezotome Cube Piezotome Solo LED	Mandible D2 Maxillary D3	1-3	80-100 ml/min

Service life

As it is not possible to establish a maximum number of uses (that may be determined by many parameters such as duration of use, hardness of tissue, the force applied, wear), we recommend that medical devices being routinely used are replaced at least once a year. Replace the medical device if the tip does not vibrate at the expected frequency, the treatment is not progressing as normal and is taking longer or is at a standstill.


Associated documentation

Document title	References
Consulting electronic user instructions	J00007
Cleaning, disinfection and sterilisation instructions for tips	J02001
Crest splitting clinical tips	J57331
Dental surgery ultrasonic generator power settings table	J58010
General instructions relating to the complete range of dental surgery tips	J87301


Sterilisation




Sterilise prior to each use




The tips must be cleaned, disinfected and sterilised prior to each use. Prior to each use, please refer to the cleaning, disinfection and sterilisation instructions for tips J02001.

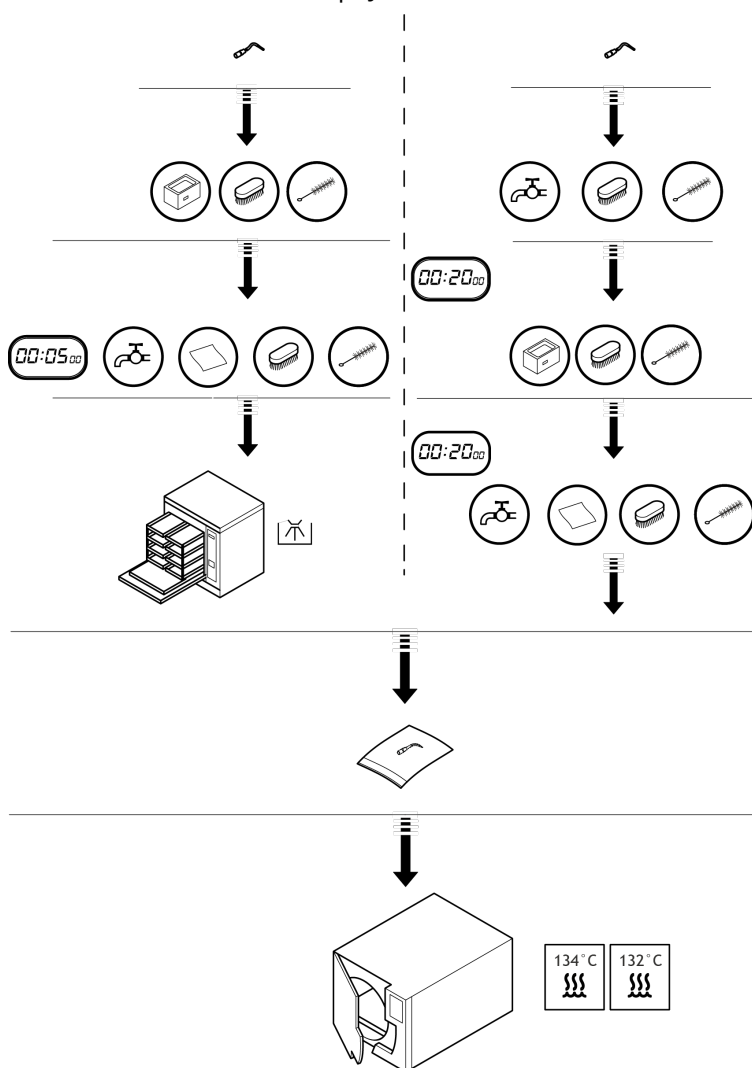

Installation

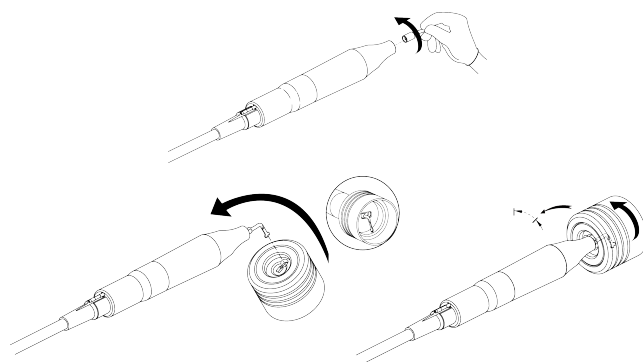

Disassembly

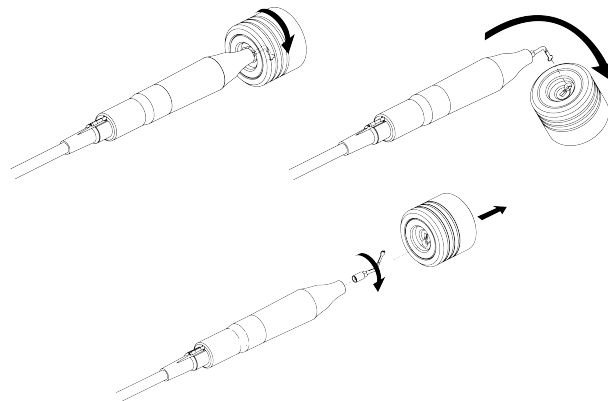

Manufacturer identification



SATELEC
A Company of ACTEON Group
17, avenue Gustave Eiffel
BP 30216
33708 MERIGNAC cedex
France
Tel. +33 (0) 556.34.06.07
Fax. +33 (0) 556.34.92.92
E.mail: satelec@acteongroup.com
www.acteongroup.com



Date of first CE marking

2011



The practitioner has to continually monitor the clinical site to immediately identify any heating risk

Tip | CS6 II | J01291 | (11) | V3 | 05/2018 | NO50EN340C

SATELEC S.A.S. | A Company of ACTEON Group
17 av. Gustave Eiffel | BP 30216 | 33708 MERIGNAC cedex | FRANCE
Tel. +33 (0) 556 34 06 07 | Fax. +33 (0) 556 34 92 92
E-mail: satelec@acteongroup.com | www.acteongroup.com

Download



Instructions For Use

